



Memorial Sloan Kettering
Cancer Center

DigITs

DIGITAL, INFORMATICS, TECHNOLOGY

Nonin 3230 Pulse Oximeter

Patient Remote Monitoring



April 2022


Overview

Your healthcare provider would like you to use a pulse oximeter to check your oxygen levels from home. This device lets your care team monitor your oxygen levels and provide help as early as possible. Please view these instructions on how to set up and take a reading using your pulse oximeter. If you have questions, please call your healthcare provider's office.

Setting up the Nonin 3230 Pulse Oximeter




Slide off the back cover of the pulse oximeter and install two AAA batteries

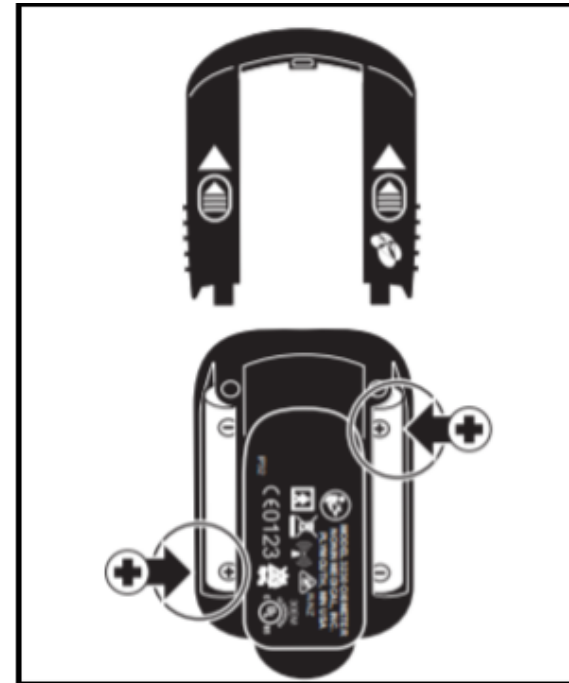

Slide the cover back on.

Your Nonin Pulse Oximeter is ready to take a reading.


How to take a reading with your Nonin 3230 Pulse Oximeter

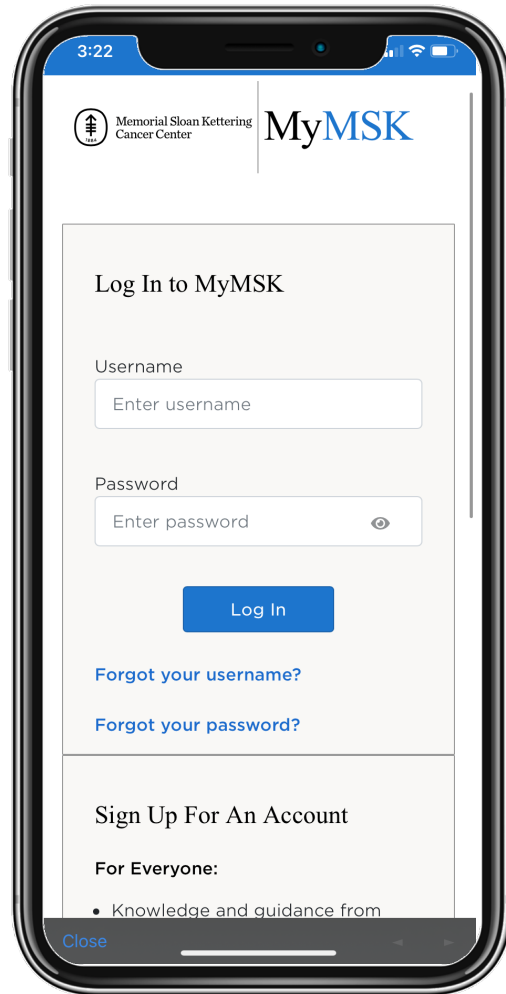


Open the MyMSK app and log in with your username and password.

How to take a reading with your Nonin 3230 Pulse Oximeter

Read the Emergency Notification and press the “x” to close it

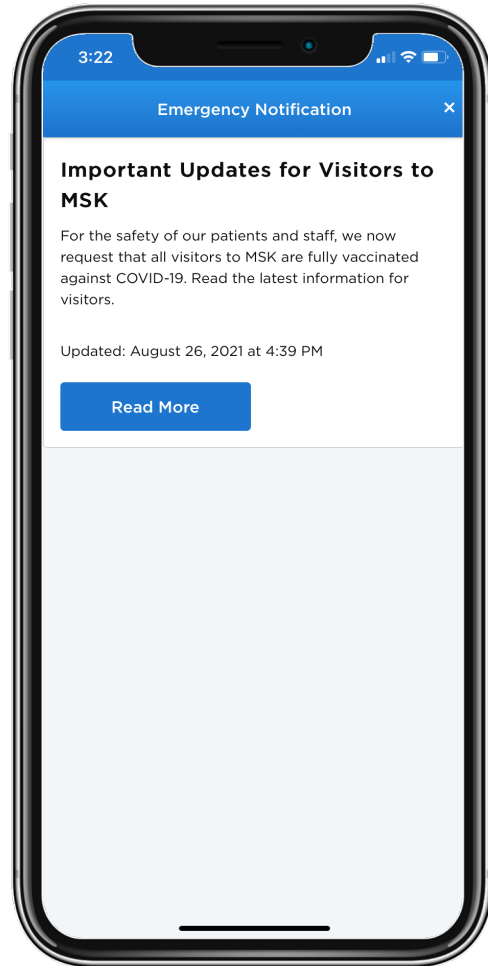


Select the Menu from the bottom

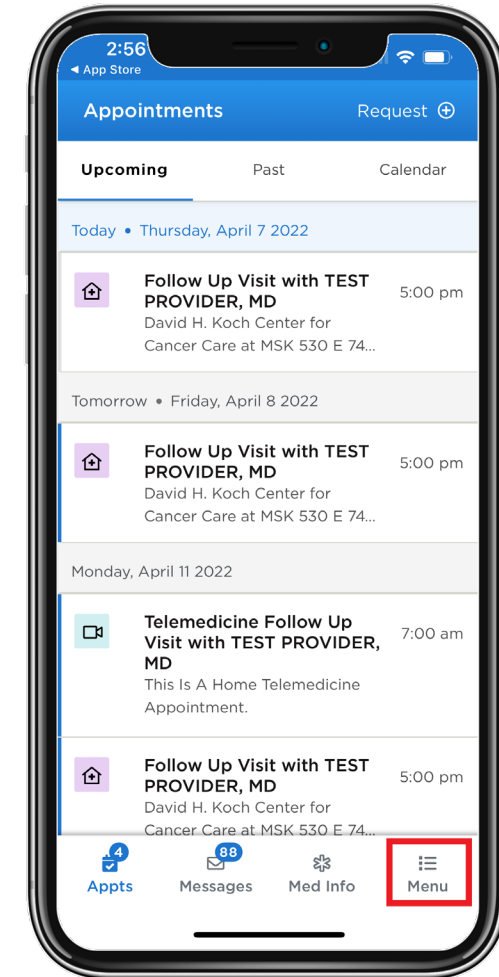


How to take a reading with your Nonin 3230 Pulse Oximeter

Select the Remote Monitoring

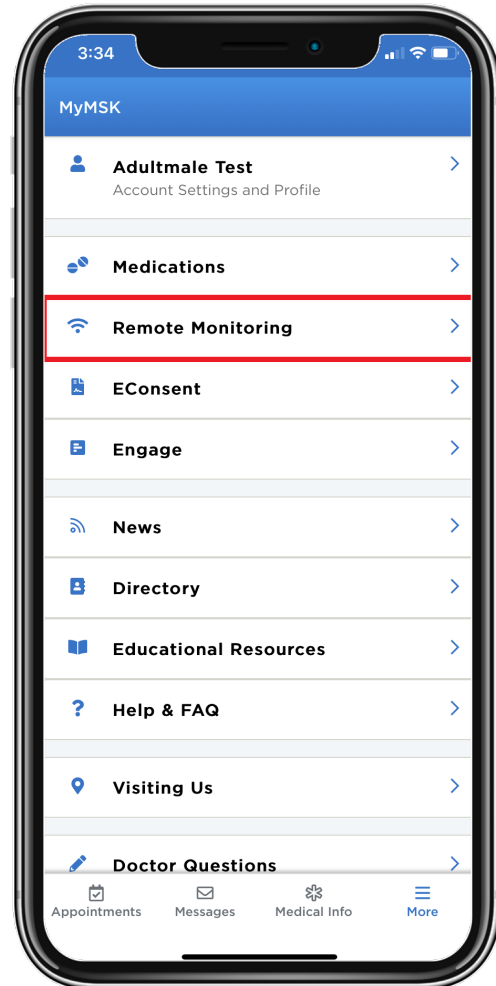

Select Nonin 3230

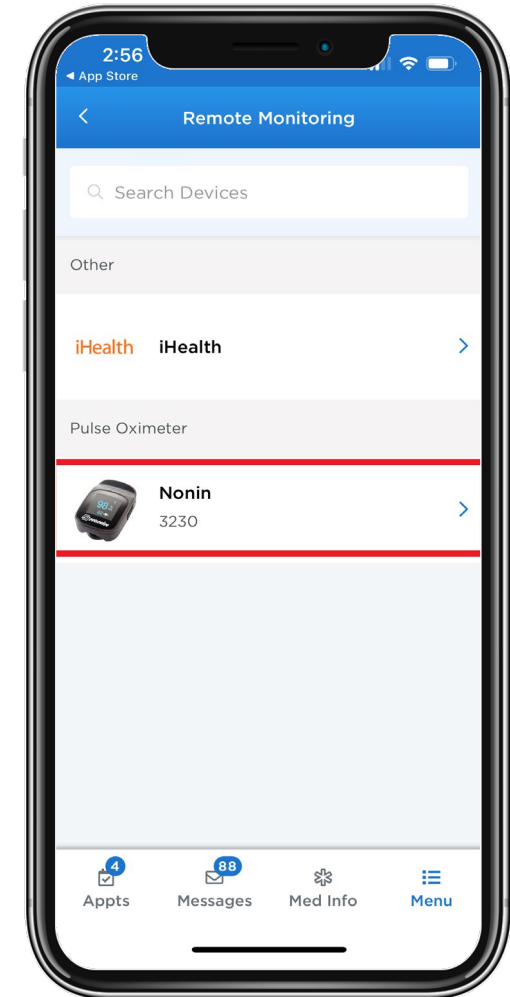


How to take a reading with your Nonin 3230 Pulse Oximeter



Put the pulse oximeter on any of your 3 middle fingers (not your thumb or pinky). The display should face you.

How to take a reading with your Nonin 3230 Pulse Oximeter

With the pulse oximeter on your finger select Get new reading

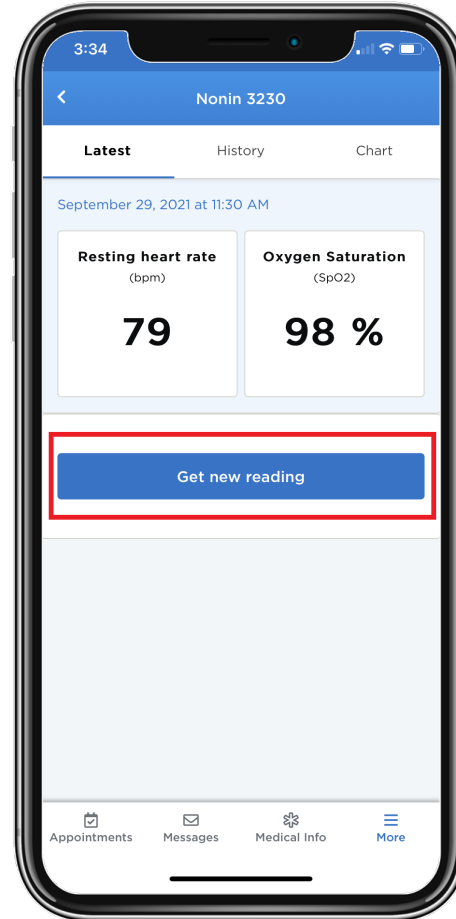


Select OK




How to take a reading with your Nonin 3230 Pulse Oximeter

Select "Pair." This connects your Nonin 3230 pulse oximeter to your phone.

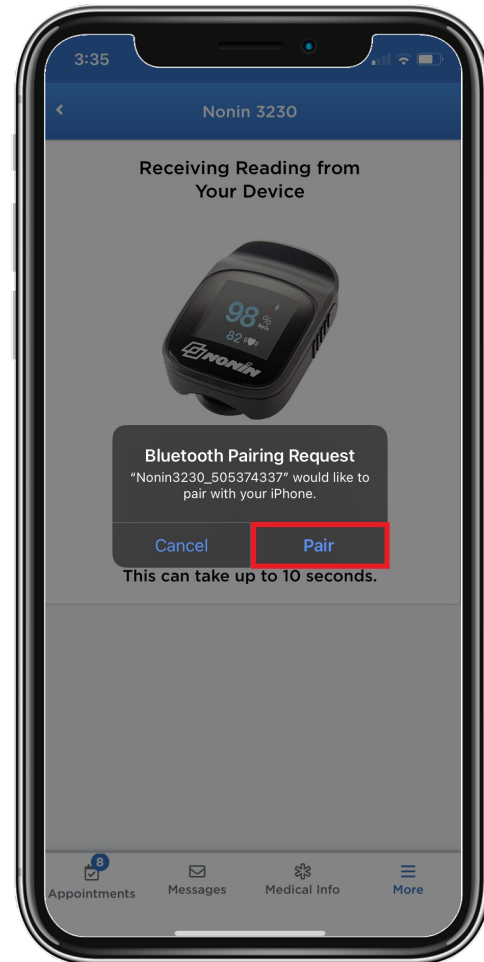


Your device will start to take a reading. This may take up to 10 seconds.

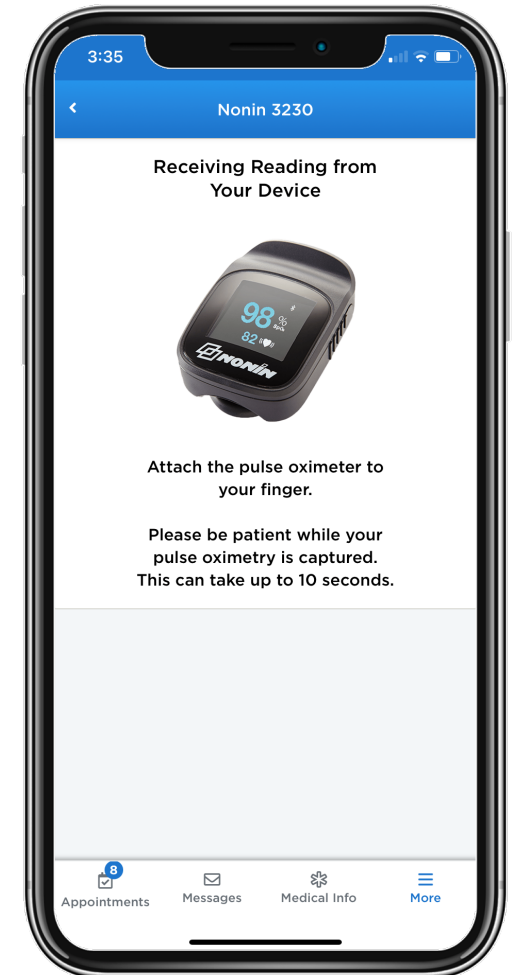


How to take a reading with your Nonin 3230 Pulse Oximeter


When you see a measurement, select “Submit.” This will send your reading to MSK.

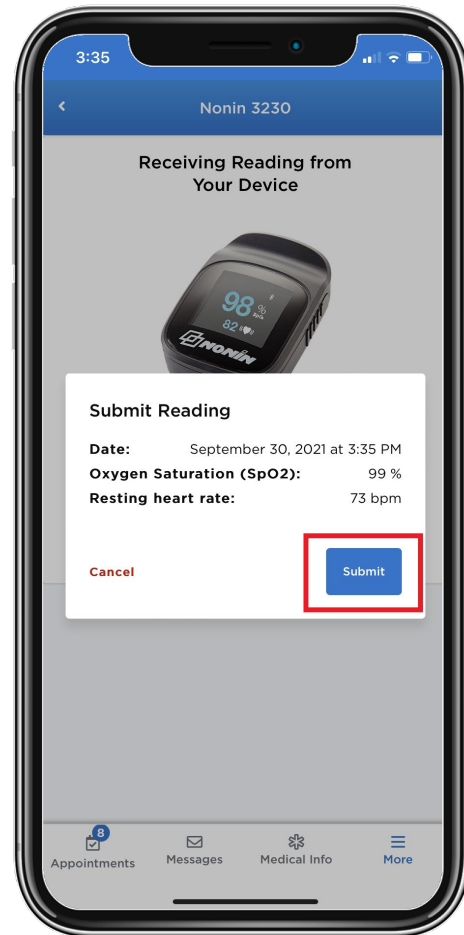

You can see your new reading on the screen. It also will be sent to your healthcare provider’s office.

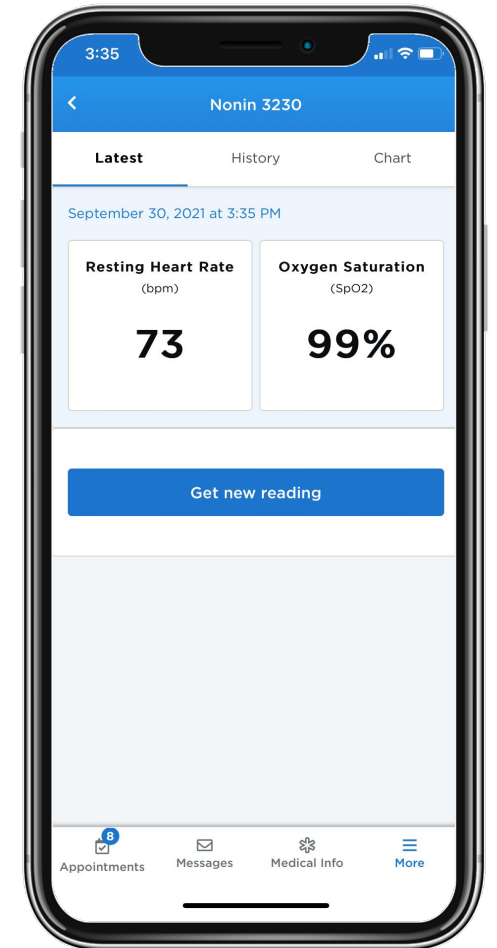

Low battery alert

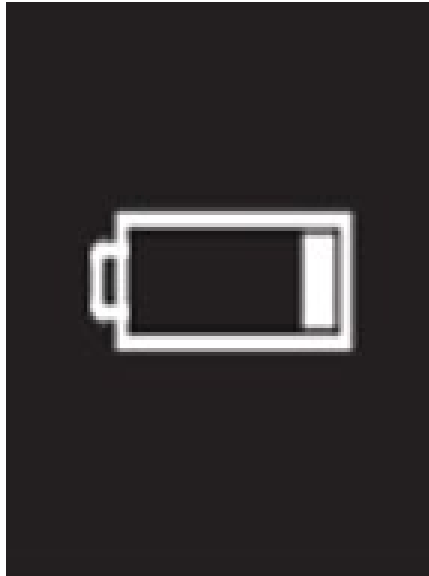

A low battery symbol will appear on the Nonin device when batteries need to be changed.

When the battery is very low, it will appear on the full screen and the device will not work. You will need to change the batteries.